




PERVAPORATION TEST SKID TECHNICAL DATA SHEET



TECHNICAL SPECIFICATION FOR PERVAPORATION TEST SKID

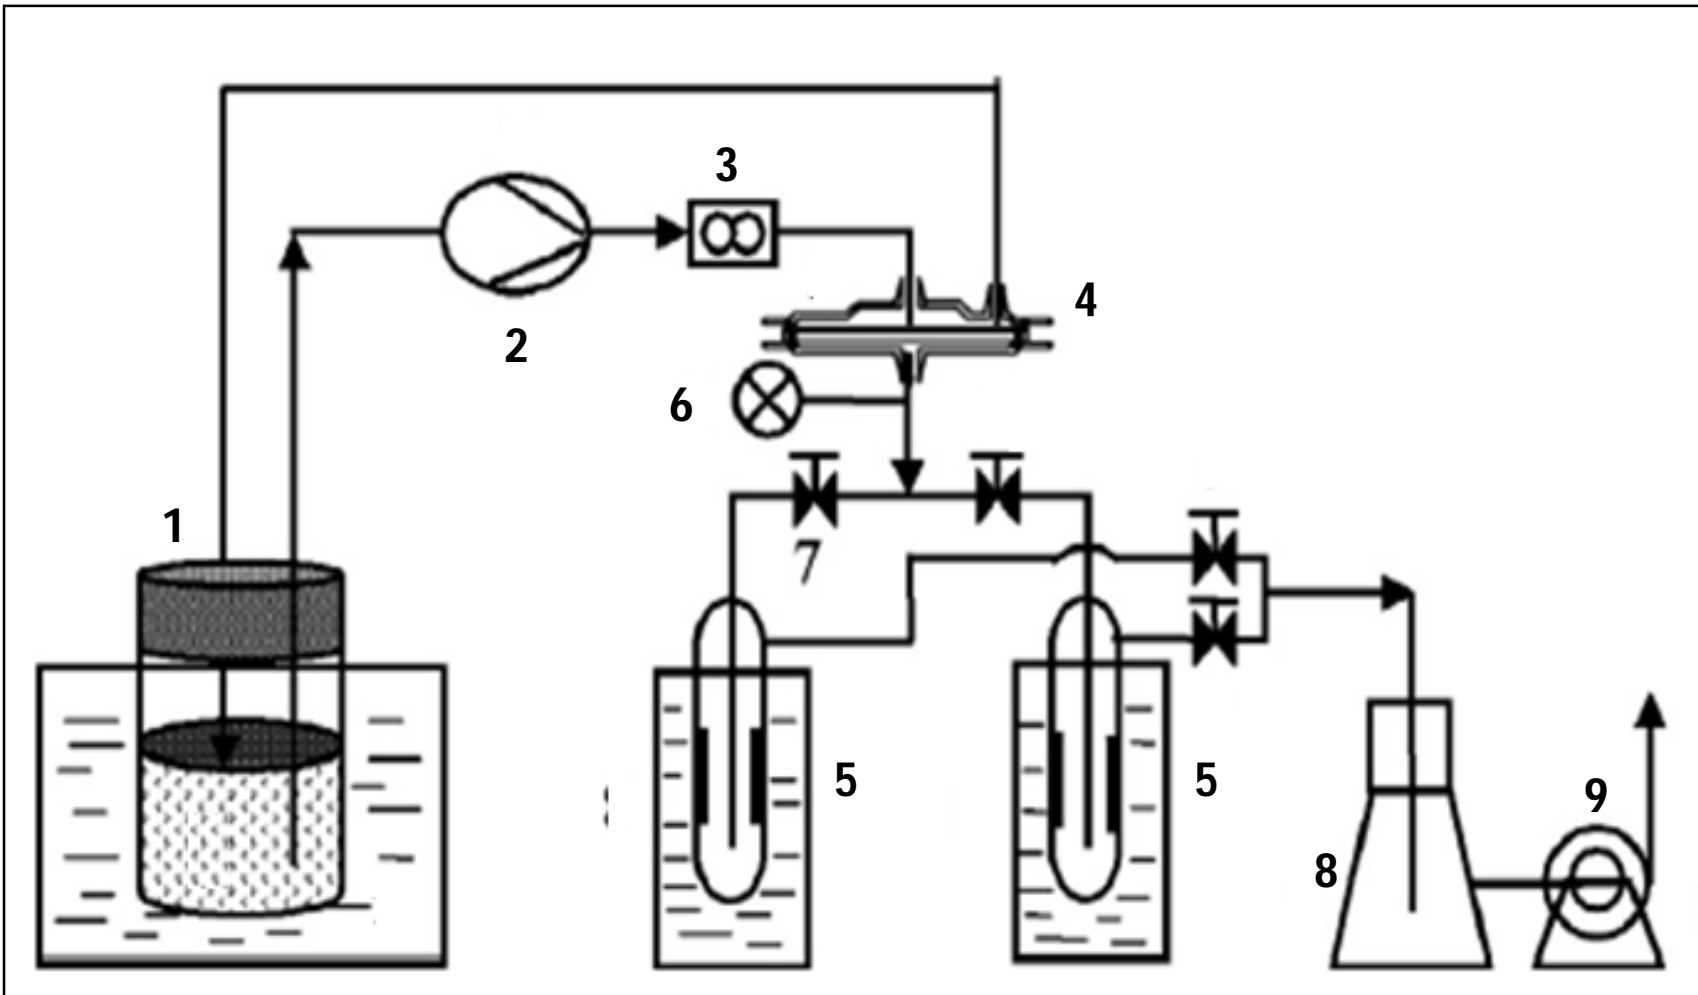

1. FEED LIQUID TANK

1 No

MOC of the Tank

: SS 304

Capacity

: 2 Ltrs

2. PERISTALTIC PUMP

1 No

Flow

0 - 10 Liters/ Hr

Input

230 V AC, 50 Hz, 3 HP

Tube

SILICONE

3. ROTA METER

1 No

Flow

2 – 20 LPH

MOC

Acrylic

4. FLAT SHEET MEMBRANE HOLDER

1 No

Type

: Circular

MOC

: SS

Size of Membrane

: 100mm Dia

5. COLD TRAP

1 No

MOC

: Glass/ SS

Capacity

: 1 ltr

6. PRESSURE GAUGE

1 No

Range

: 0 – 2.5 Kg/cm²

MOC

: SS

Type

: Bourden Tube

7. CONTROL VALVES

1 Set

MOC

: SS

8. VACCUM TANK

1 No

MOC

: SS

Capacity

: 1 Ltr

9. VACCUM PUMP

1 No

Flow

: 50 lph

Vaccum

: -500 mmWc

M/s TECH INC

NO 32, INDIAN BANK COLONY III MAIN, AMBATTUR, CHENNAI 600053

Ph: 044-265284142 ; Mob:9790917184 Email: techincmail@gmail.com